

# OneFit ORDER FORM

## Order details

Clinic

Prosthetist

Patient/User ref.

Previous cover (s/n)

Notes

## Common details

Design

Material

Firm

Flex

Prosthesis

AK/ TF

Coating

Glossy

Matte

Attachment

Magnets &  
Fast-clamp

Magnets &  
C-Clamp

Screws &  
C-Clamp

Rotator  
adapter

Yes

No

Socket  
trimline

Front/Back  
(only Firm)

Wrapped

Colors

Global

Front

Back

Base

Detail

Extras

Engrave (Firm/Flex)

Size  
reduction

0 %

Vinyl (Firm)

5 %


10 %

## Measuring

Follow the instructions in the next page and fill in the requested measurements.


# OneFit - Scanning Ordering

## 4 photos sound leg

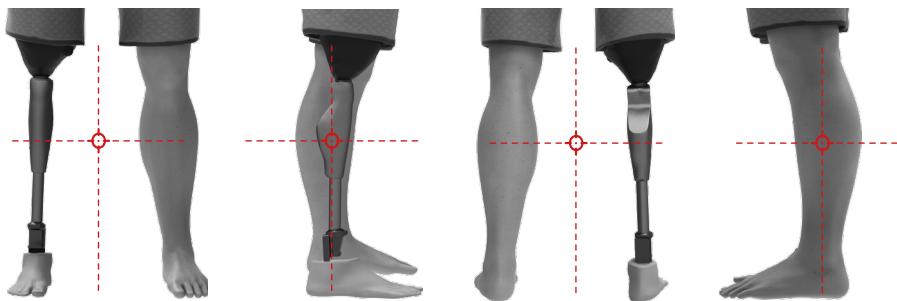


Take 4 photos of the user wearing the prosthesis, as shown in the images above. The camera must be placed perpendicular to the legs, in a low position, and both legs must be centered on the photo. Please remember that all prosthetic components must be completely visible, including the socket. Please remove shoes, socks and any object that covers the prosthesis.

## 3 measurements

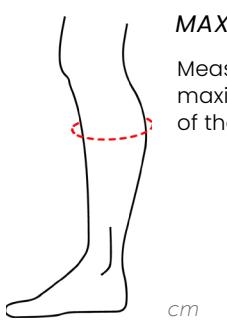


### MAX CALF VOLUME

Measure the maximum volume of the calf.

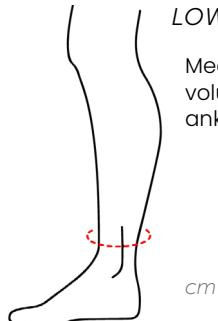

### LOW CALF VOLUME

Measure the volume at the ankle bone.

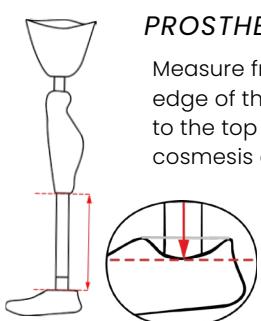


### PROSTHESIS LENGTH

Measure from the bottom edge of the prosthetic knee to the top edge of the foot cosmesis on its lowest part.


## Scanning




COMPLETE PROSTHESIS

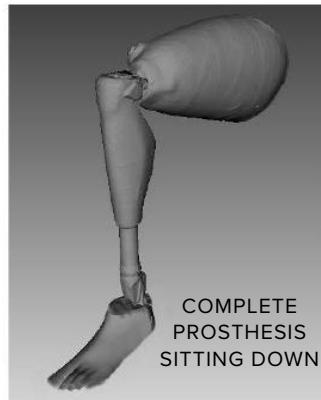

COMPLETE PROSTHESIS SITTING DOWN

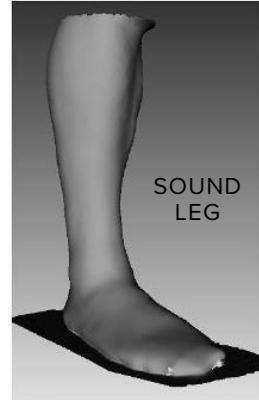

SOUND LEG

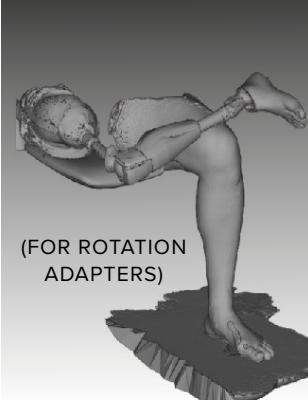

(FOR ROTATION ADAPTERS)

- Scan the complete prosthesis and the sound leg, with the patient standing and seated. If a rotation adapter is present, also scan the prosthesis in the position shown (prosthesis resting on the sound knee). You can scan both legs in the same file or separately.
- All prosthetic components should be clearly visible on the scan, including the lower part of the socket. Please remove any item that covers the prosthesis (sock, foam, other coverings ...)
- No reflecting ground: Avoid problems with reflective material or dark areas. If your scanner does not receive information from these areas, cover the reflective parts or dark areas with matt tape, tightly taped to the surface so that it does not create extra bulk.
- We recommend that the environment contrasts in color with the prosthesis.
- Set the scanner to the highest resolution possible.

Recomended scanner: Einstar Scanner; Shining 3D Einscan Pro Series Hand Scanners; Artec Structured Light Hand Scanners; Creaform Hand Scanners; Peel3d 3D Scanner.

Not recommended scanners: 3D Systems / Cubify Sense; Structure Sensor / Core; Microsoft Kinect 3D Scanner; Intel Infrared Sensor Scanners

## SEND US THE FILES AND FORM

Send us this guide with the order details, measurements and photos to [orders@unyq.com](mailto:orders@unyq.com). If you need further assistance please contact us at [orders@unyq.com](mailto:orders@unyq.com) or +34 854 85 60 92